



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 20TM1646

Page.: 1 of 3

Certificate of Calibration

Equipment : Incubator

Manufacturer : Sanden Intercool

Model : SRC-680SRTM

Serial No. : SRC680201-1107-00166

ID No. : CHI-003

Submitted by : Environment & Laboratory Co.,Ltd.
40 Soi Liangmueangnonthaburi 13
Talad Kwan, Mueang,
Nonthaburi 11000

Location : Room No. 301

Received Order : 19 August 2020

Calibration Date : 20 August 2020

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Kunchit Promprat

Approved by :

Malee

Approved Signatory

- () Pornthippa Tameyakul
(✓) Malee Butkruea
() Suwit Imjai

Issue Date : 26 August 2020

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Incubator
 Condition As-Received : Used Item
 Reference : 2008-0401OC-3

Cert. No.: 20TM1646

Page.: 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY44067817	20LM8	NIST, NIMT	29 Jul 2021

2. This certification is traceable to the SI unit.

3. This certificate is valid only to the item calibrated on date and place of calibration.

Remark : NIST : National Institute of Standards and Technology, The United State of America.

NIMT : National Institute of Metrology Thailand.


Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available

Environment during calibration		
	Beginning	Finished
Temp. (°C)	28	28
REL.Humi. (%)	56	63
AC Supply (Volt)	220	220

Position :	Ref. Std./ID No.:
1	19-15RTD-01
2	19-15RTD-02
3	19-15RTD-03
4	19-15RTD-04
5	19-15RTD-05
6	19-15RTD-06
7	19-15RTD-07
8	19-15RTD-08
9 (ref.)	19-15RTD-09
10	19-15RTD-10
11	15RTD2/11
12	15RTD2/12
13	15RTD2/13

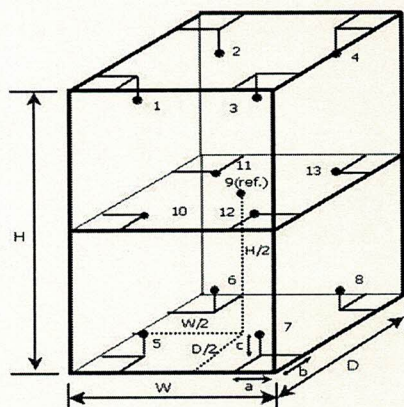

Dimension of Chamber :

D = 0.60 m
 W = 0.70 m
 H = 1.2 m
 Capacity = 0.50 m³

Probe Installation Details :

a = 10 cm
 b = 10 cm
 c = 10 cm

Malu.



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2008-0401OC-3
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 20TM1646
Page.: 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
20.0	20.2	20.2	0.16	0.24	0.54	0.30	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
20.0	1	2	3	4	5	6	7	8	9 (ref.)
	20.266	20.259	20.104	20.053	20.404	20.087	20.249	20.329	20.254
	10	11	12	13					
	20.280	20.276	20.123	20.264					

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu